

# Report - 10890513 - Alarm

## Report Created by

Name: Jon Lockwood

Company: HOBO Data Loggers

Email: jon.lockwood@onetemp.com.au

## Report Information

Report Date: 04/08/2016 13:15:06 ACST

Start Date: 03/08/2016 06:25:00 ACDT

Deployment Name: Vaccine Fridge 1

Download Date: 03/11/2016 08:53:21 ACDT

Logger Model: CX402

Logging Interval: 5m

Serial Number: 10890513

Total Data Points: 894

## Alarm Information

Alarms During Deployment: **YES**

Number of High Alarms: 1

High Alarm Limit: 8 °C

Number of Low Alarms: 0


Low Alarm Limit: 2 °C

Number of Probe Disconnects: 1

Duration: Alarm after 30m consecutive samples

Elapsed Time Outside Alarm Limits: 5h

Elapsed Time Probe Disconnected: 15m

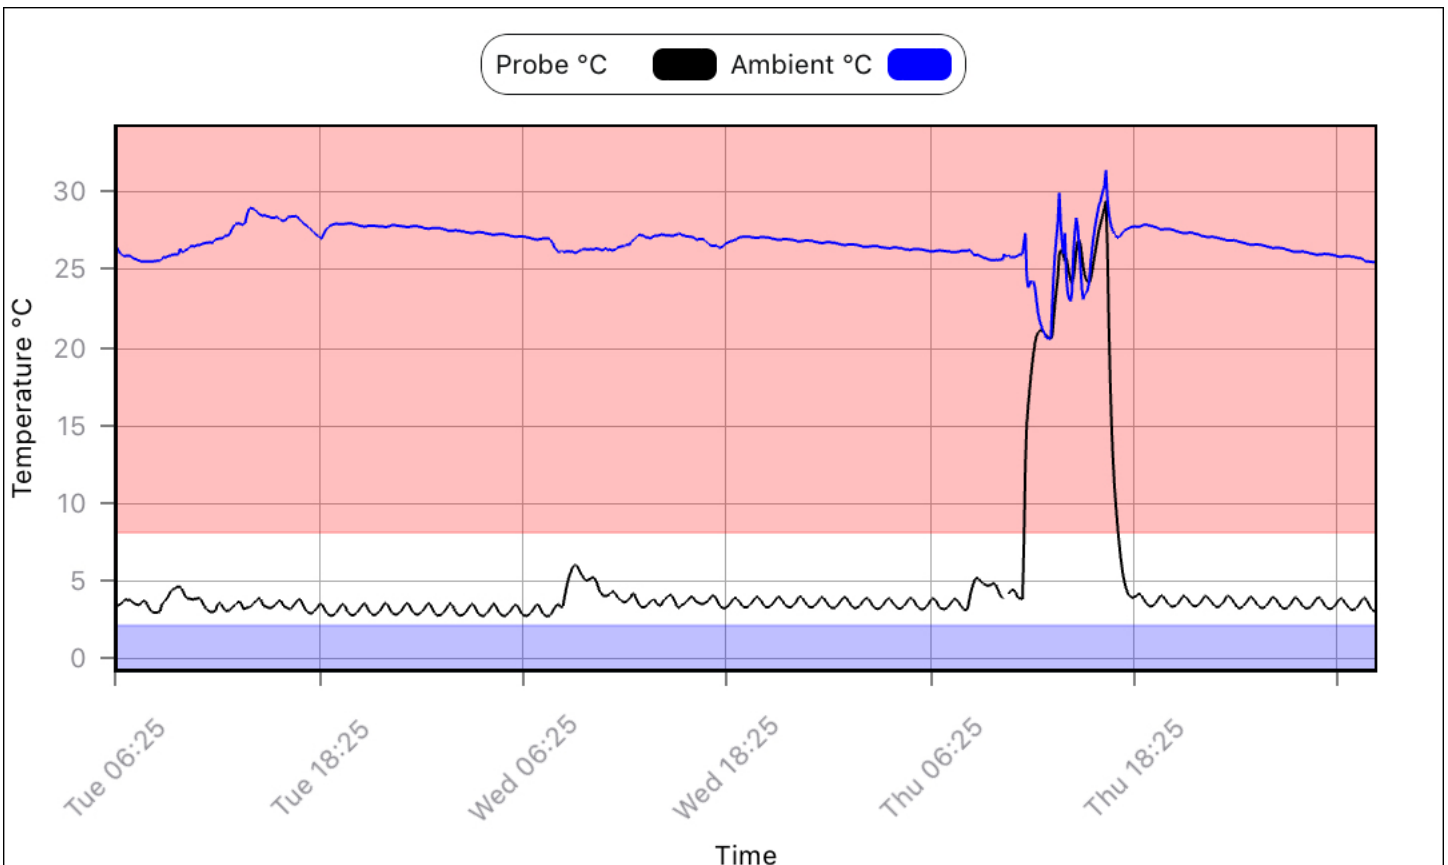

Deployment Statistics		
Statistic	Probe °C	Ambient °C
Minimum Temperature	2.61	20.48
Maximum Temperature	29.36	31.33
Average / Mean Temperature	4.88	26.68
Standard Deviation	5.16	1.12
Mean Kinetic Temperature	4.79	26.68

Note: Probe disconnects may invalidate mean kinetic temperature values

Audit Report Table - Australia/Adelaide				
Date Time	Event	User	Latitude	Longitude
2016-03-08 6:25:00	Started	jon.lockwood@onetemp.com.au	-34.942	138.570
2016-03-08 7:09:26	Check Performed	jon.lockwood@onetemp.com.au	-34.942	138.570
2016-03-08 9:07:18	Downloaded	duane.callaghan@onetemp.com.au	-34.942	138.569
2016-03-08 9:10:22	Downloaded	duane.callaghan@onetemp.com.au	-34.942	138.569
2016-03-08 9:12:20	Downloaded	duane.callaghan@onetemp.com.au	-34.942	138.570
2016-03-08 10:26:19	Downloaded	graeme.allen@onetemp.com.au	-34.942	138.570
2016-03-08 23:59:59	Missed Check	--	--	--
2016-03-09 11:59:59	Missed Check	--	--	--
2016-03-09 15:37:34	Downloaded	graeme.allen@onetemp.com.au	-34.942	138.571
2016-03-10 0:00:00	Missed Check	--	--	--
2016-03-10 9:11:31	Check Performed	duane.callaghan@onetemp.com.au	-34.942	138.570
2016-03-10 10:54:07	Downloaded	duane.callaghan@onetemp.com.au	-34.942	138.570
2016-03-10 13:34:43	Downloaded	duane.callaghan@onetemp.com.au	-34.793	138.693
2016-03-10 16:51:53	Downloaded	duane.callaghan@onetemp.com.au	-34.942	138.570
2016-03-10 16:54:01	Check Performed	duane.callaghan@onetemp.com.au	-34.942	138.570
2016-03-11 8:53:19	Downloaded	jon.lockwood@onetemp.com.au	-34.942	138.570

Daily Statistics - Australia/Adelaide			
Date	Daily Minimum Temp, °C	Daily Maximum Temp, °C	Daily Average Temp, °C
2016-03-08	2.64	4.51	3.28
2016-03-09	2.61	5.92	3.47
2016-03-10	3.01	29.36	8.05
2016-03-11	2.93	3.93	3.41

## Alarm Report - Date Time, Australia/Adelaide

Start	End	Type	Duration	Max/Min Temp, °C	Ambient Temp, °C
2016-03-10 10:50:00	2016-03-10 11:05:00	Probe Disconn	15m	--	--
2016-03-10 12:35:00	2016-03-10 17:35:00	High Alarm	5h	29.36	24.15